


Determining the heating up time and cooling down time

DIN 12880:2007-05 stipulates that the **heating up time** is considered to be finished as soon as the **actual temperature** at the centre of the chamber remains permanently within the limits specified in the standard.

[Overview Glossary Temperature control chamber](#)

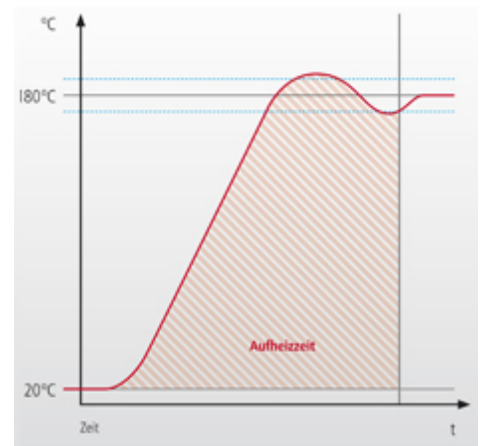

End of the heating up time (DIN 12880:2007-05)

Autor:

www.atmosafe.net > [Glossary](#) > [DIN 12880:2007-05](#) > [Heating up time](#)

AtmoSAFE is a brand of Memmert GmbH + Co. KG
Copyright © 2009 Memmert GmbH + Co. KG.
All Rights Reserved.



memmert
Experts in Thermostatics